

Pantera Pro

Semi-Compliant Workhorse Balloon

Indicated for dilatation of coronary artery
or bypass graft stenosis



- Outstanding crossability in tight lesions¹
- 43 % less friction² during kissing balloon technique
- 38 % more push³ to reach target lesion

¹ 1.25 - 2.0 mm diameter, when compared to key competitors. BIOTRONIK data on file

² vs Trek (Abbott), BIOTRONIK data on file

³ vs Mini Trek (Abbott), BIOTRONIK data on file


Pantera Pro

Excels in challenging cases

Challenging lesions require a versatile workhorse balloon. Be it a tight lesion or a complex bifurcation, Pantera Pro offers the performance to reach, cross and dilate.

Outstanding crossability in tight lesions¹


The proprietary balloon material for small sizes enables slim balloon shoulders while maintaining durability. Coupled with the newly hydrophilic balloon coating, Pantera Pro excels in tight lesions.

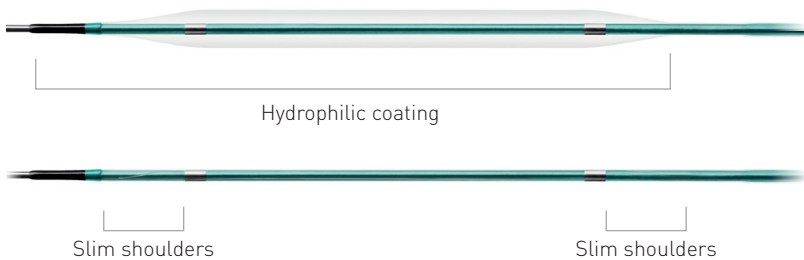

43 % less friction² during kissing balloon technique

The reduced distal shaft profile lowers friction when using two balloons in a 6F guiding catheter.*

Lowest friction during Kissing Balloon Technique compared to main competitors

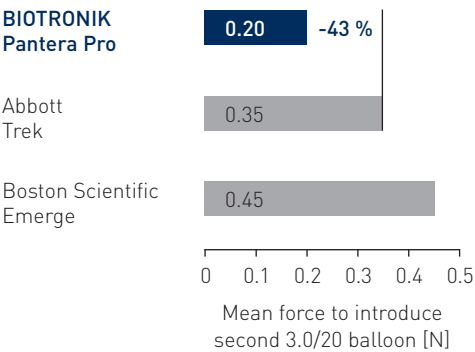

* Any combination of two diameters not larger than 3.5 mm within a 6F guiding catheter with a minimal inner diameter of 0.070"/1.78 mm.


Superior pushability

Excellent visibility thanks to platinum-iridium markers


38 % more push³ to reach target lesion

BIOTRONIK's unique Enhanced Force Transmission shaft delivers optimal pushability due to the direct transition from proximal metallic hypotube to distal guide wire support section.


Pantera Pro

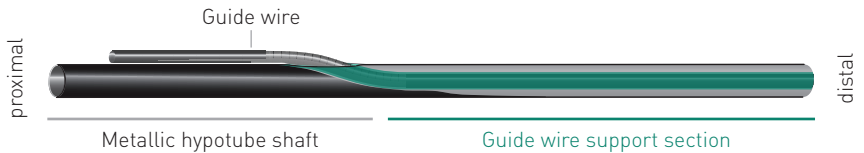

Competitors

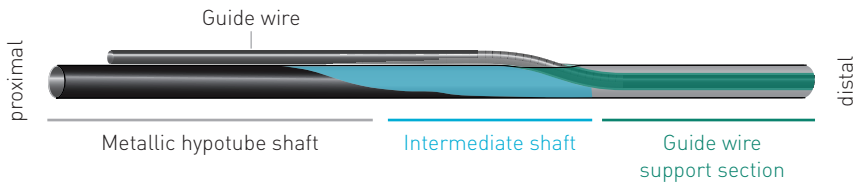

Superior pushability compared to main competitors

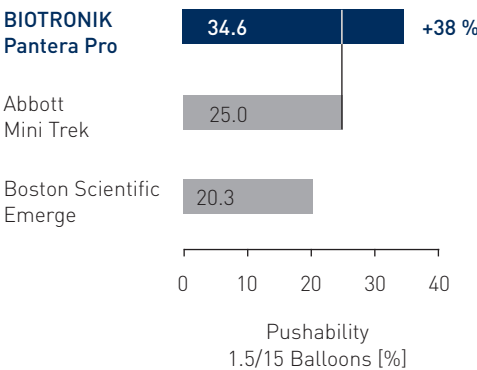

Pantera Pro

Semi-Compliant Workhorse Balloon

Technical Data	Proximal shaft	
	Design	Hypotube design
	Diameter	2.0F
	Shaft markers	92 cm and 102 cm from tip
	Distal shaft	
	Guiding catheter	5F (min. I.D. 0.056" / 1.42mm)
	Guide wire diameter	0.014"
	Lesion entry profile	0.017"
	Usable length	140 cm
	Balloon material	Semi Crystalline Co-Polymer
	Balloon folding	ø 1.25 - 1.5 mm: Two-fold; ø 2.0 - 4.0 mm: Tri-fold
	Balloon markers	Platinum-Iridium: ø 1.25 - 1.5 mm one marker; ø 2.0 - 4.0 mm two markers
	Coating distal shaft	Hydrophilic (end of balloon to Guide Wire (GW) exit port)
	Balloon and tip coating	ø 1.25 - 2.0 mm: Hydrophilic ø 2.50 - 4.0 mm: Hydrophobic
	Kissing balloon technique	6F guiding catheter (min. I.D. 0.070"/1.78 mm), up to ø 3.5 mm
	Diameter	2.6F (ø 1.25 - 2.0 mm); 2.7F (ø 2.5 - 3.5 mm); 2.9F (ø 4.0 mm)

Compliance Chart		Balloon diameter x length (mm)						
		ø 1.25 x 6-20	ø 1.50 x 6-20	ø 2.00 x 10-30	ø 2.50 x 10-30	ø 3.00 x 10-30	ø 3.50 x 10-30	ø 4.00 x 10-30
Nominal Pressure (NP)	atm*	7	7	7	7	7	7	7
	ø (mm)	1.24	1.49	2.01	2.49	3.08	3.62	3.95
Rated Burst Pressure (RBP)	atm*	14	14	14	14	14	14	14
	ø (mm)	1.37	1.72	2.23	2.93	3.50	4.06	4.55

*1 atm = 1.013 bar

Ordering Information		Balloon ø (mm)	Catheter length 140 cm Balloon length (mm)					
			6	10	15	20	25	30
5F	1.25	393289	393291	393298	393305	–	–	–
	1.50	393290	393292	393299	393306	–	–	–
	2.00	–	393293	393300	393307	393312	393317	–
	2.50	–	393294	393301	393308	393313	393318	–
	3.00	–	393295	393302	393309	393314	393319	–
	3.50	–	393296	393303	393310	393315	393320	–
	4.00	–	393297	393304	393311	393316	393321	–

Pantera Pro is part of the BIOTRONIK coronary solutions portfolio, including:

- Stents: **Orsiro**, **PRO-Kinetic Energy**, **PK Papyrus** ■ Balloons: **Pantera LE0**, **Pantera Lux**
- Guide Wires: **Galeo Pro**, **Cruiser**, **Magnum**

For ordering please contact your
local sales representative

BIOTRONIK AG
Ackerstrasse 6
8180 Bülach · Switzerland
Tel +41 (0)44 8645111
Fax +41 (0)44 8645005
info.vi@biotronik.com
www.biotronik.com